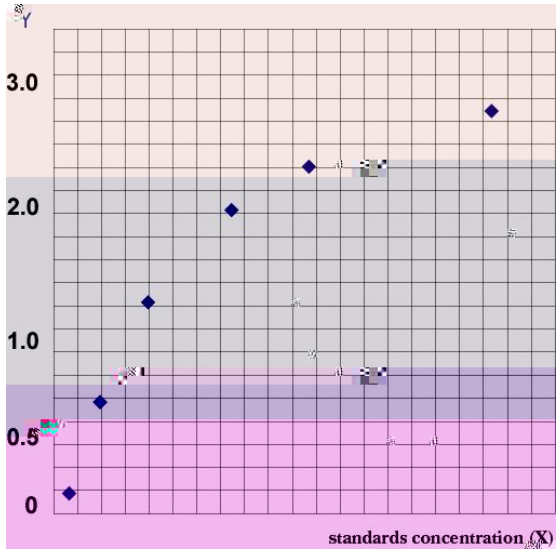
	*	*	
–			

–


Y
3.0
2.0
1.0
0.5
0
standards concentration (X)

This GA ELISA kit is intended Laboratory for Research use only and is not for use in diagnostic or therapeutic procedures.


1. Do not substitute reagents from one kit to another. Standard, conjugate and microplates are matched for optimal performance. Use only the reagents supplied by manufacturer.
2. Do not remove microplate from the storage bag until needed. Unused strips should be stored at 2-8ÁC in their pouch with the desiccant provided.
3. Mix all reagents before using.

Remove all kit reagents from refrigerator and allow them to reach room temperature (20-25ÁC)

Name	96 determinations	48 determinations
Microelisa stripplate	12*8strips	12*4strips
Standard	0.3ml*6tubes	0.3ml*6tubes
Sample Diluent	6.0ml	3.0ml
HRP-Conjugate reagent	10.0ml	5.0ml
20X Wash solution	25ml	15ml
Chromogen Solution A	*Þ] Ď Ů	

Sealed bags	1	1

Standard (S0 Ÿ S5) concentration was followed by: 0,7.5,15,30,60,120 pmol/L

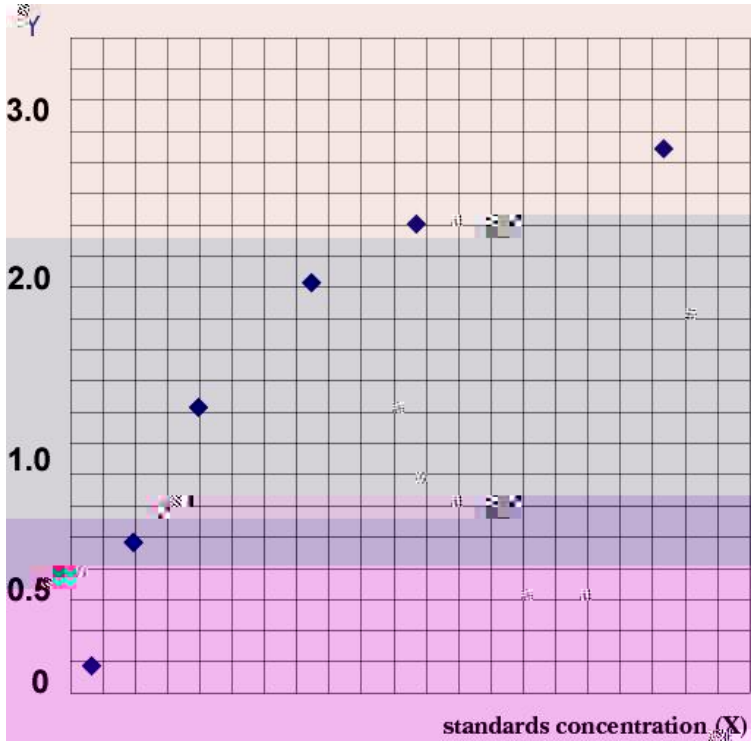

Storage 2-8 .
validity six months.